


**International Acceptance of the Nonradioactive LLNA: BrdU-ELISA for Evaluating
Allergic Contact Dermatitis Hazards**

A Jacobs¹, J Matheson², V Malshet¹, J Toy¹, J Strickland³, D Allen³, T Burns³, F Stack³,
W Stokes⁴

¹U.S. FDA, Silver Spring, MD, USA; ²U.S. CPSC, Bethesda, MD, USA; ³ILS, Inc., RTP,
NC, USA; ⁴NICEATM/NIEHS/NIH/HHS, RTP, NC, USA

Introduction


- The murine local lymph node assay (LLNA) is a test method for assessing the potential of substances to cause allergic contact dermatitis (ACD). ACD is an allergic skin reaction characterized by redness, swelling, and itching that can result from repeated contact with a sensitizing substance.
- In response to a nomination by the U.S. Consumer Product Safety Commission in 2007, NICEATM evaluated the nonradioactive LLNA: BrdU-ELISA (**Figure 1**) to assess the ACD hazard potential of substances.
- Takeyoshi et al. developed the LLNA: BrdU-ELISA (Takeyoshi et al. 2001).
 - Measures BrdU incorporation in draining auricular lymph nodes as a measure of lymph node cell proliferation.
- ICCVAM published recommendations on the LLNA: BrdU-ELISA in a test method evaluation report (available on the NICEATM–ICCVAM Web site at:
<http://iccvam.niehs.nih.gov/methods/immunotox/llna-ELISA/TMER.htm>).

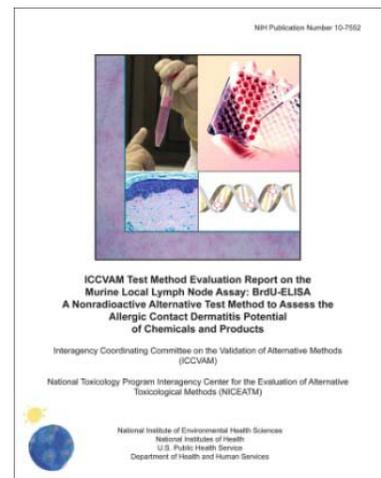

LLNA: BrdU-ELISA Test Method Protocol

- The LLNA: BrdU-ELISA protocol (**Figure 1**) is the same as the traditional LLNA protocol except:
 - It measures BrdU incorporation into lymph node cells via ELISA as a measure of proliferation (instead of ³H-thymidine via scintillation counter in the traditional LLNA)
 - BrdU is injected intraperitoneally instead of intravenously through the tail vein
- The reduced LLNA: BrdU-ELISA (rLLNA: BrdU-ELISA) should be considered and used to determine the ACD hazard potential of chemicals and products in testing situations where dose-response information is not required, or negative results are anticipated.
 - Like the reduced LLNA (ESAC 2007; ICCVAM 2009; Kimber et al. 2006), the rLLNA: BrdU-ELISA protocol uses only the high dose and thereby reduces animal use by up to 40%.
 - If existing information suggests a substance might have ACD hazard potential *and* dose-response information is needed, consider testing in the multidose LLNA: BrdU-ELISA.

Figure 1 LLNA: BrdU-ELISA Test Method Protocol

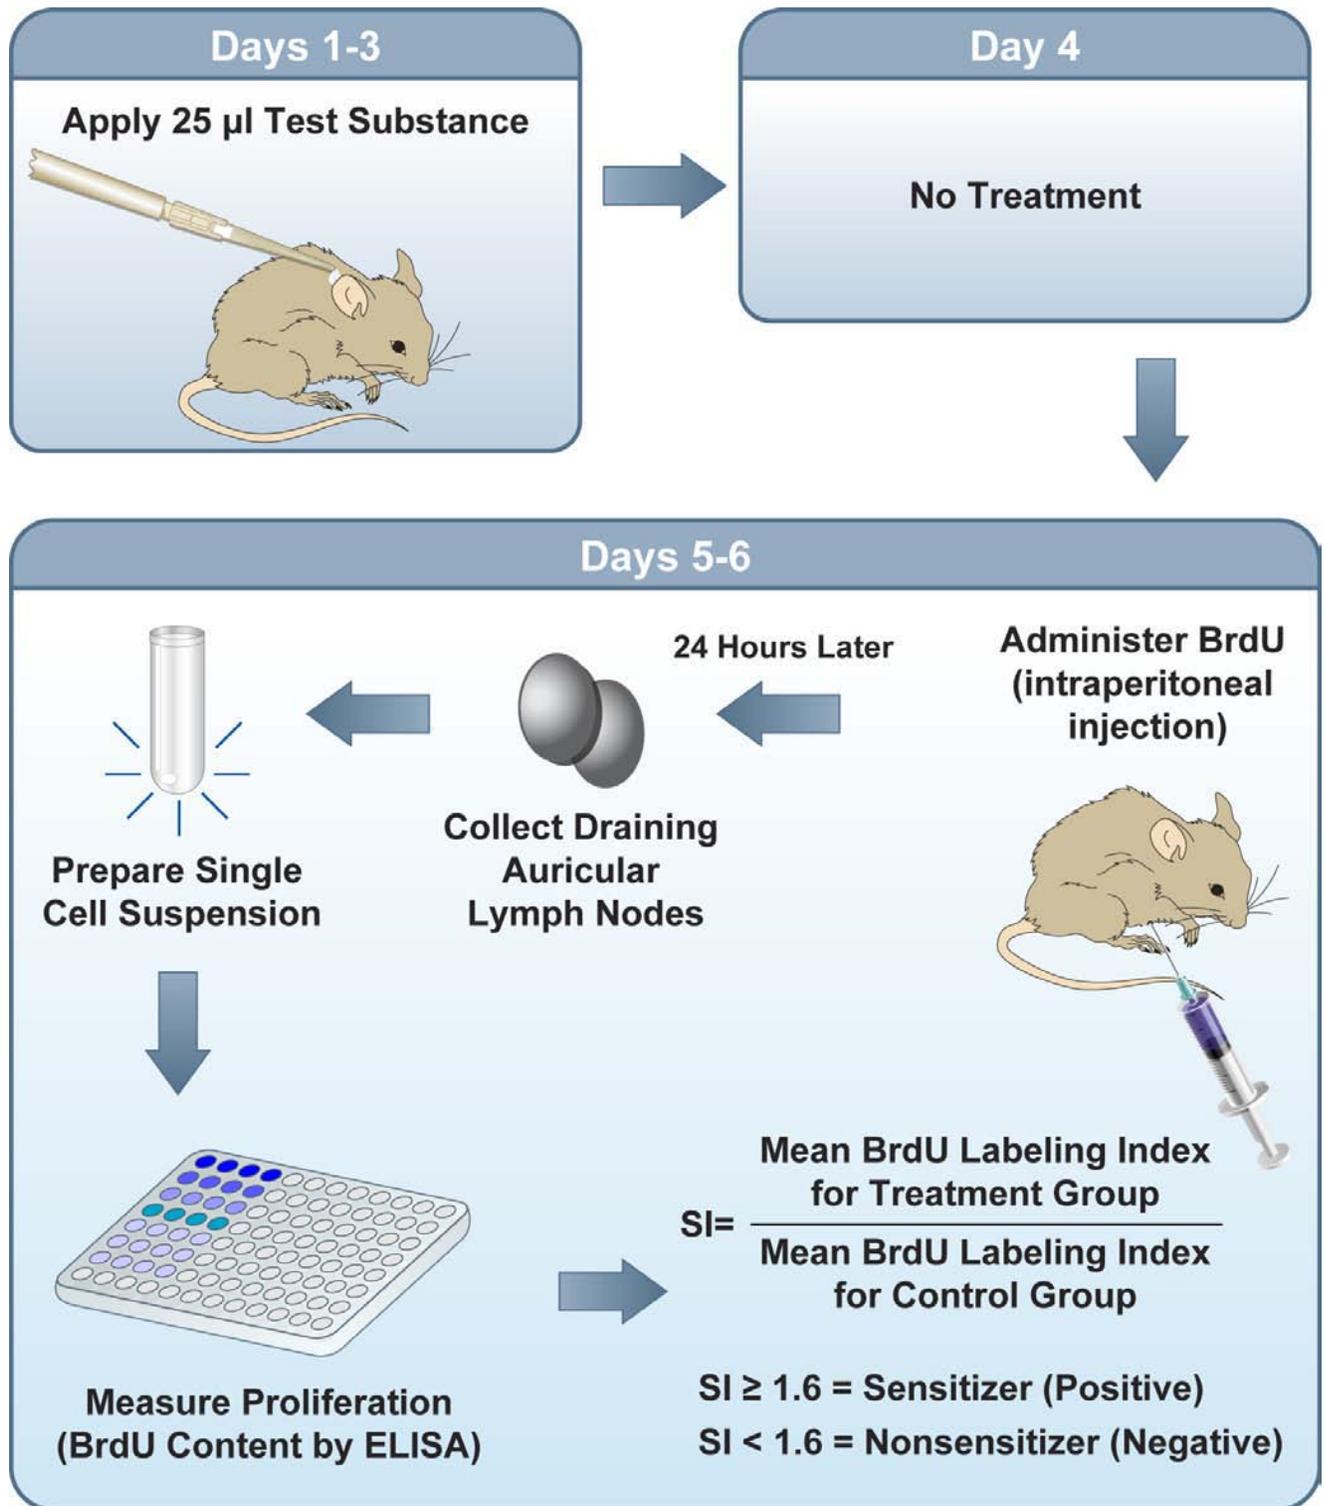

Abbreviations: SI = stimulation index

Current Validation Status of the LLNA: BrdU-ELISA

Accuracy


- Accuracy was assessed using a LLNA: BrdU-ELISA database of 43 substances.
 - Kojima et al. 2008 (interlaboratory validation study)
 - Takeyoshi et al. 2003; 2004a and b; 2005; 2006; 2007, and unpublished data
- Results compared to traditional LLNA data.
- LLNA: BrdU-ELISA results were compared to traditional LLNA data.
- Stimulation index (SI) ≥ 1.6 produced optimal results based on no false negatives (**Figure 2**).
- LLNA: BrdU-ELISA correctly identified all 32 LLNA sensitizers and 9/11 LLNA nonsensitizers.
 - Accuracy = 95% (41/43)
 - False positive rate = 18% (2/11)
 - Hexane and lactic acid: $1.6 < SI < 1.9$
 - False negative rate = 0% (0/32)

Reliability

- Determined extent of agreement of LLNA: BrdU-ELISA outcomes for 18 substances (13 LLNA sensitizers and 5 LLNA nonsensitizers) with multiple test results (intra- and interlaboratory comparisons included).
 - Complete agreement for 85% (11/13) of the sensitizer outcomes.

- Two substances (hydroxycitronellal and linalool) produced $SI < 1.6$ in one test and $SI > 1.6$ in another test.
- Complete agreement for 80% (4/5) of the nonsensitizer outcomes.
- Two substances with concordant results were false positive in LLNA: BrdU-ELISA: hexane (2/2 tests had $SI \geq 1.6$) and lactic acid (3/3 tests had $SI \geq 1.6$).
- 71% (5/7) agreement for the discordant nonsensitizer (isopropanol).

Figure 2 SI Decision Criteria Performance of the LLNA: BrdU-ELISA Compared With the Traditional LLNA Using 43 Substances


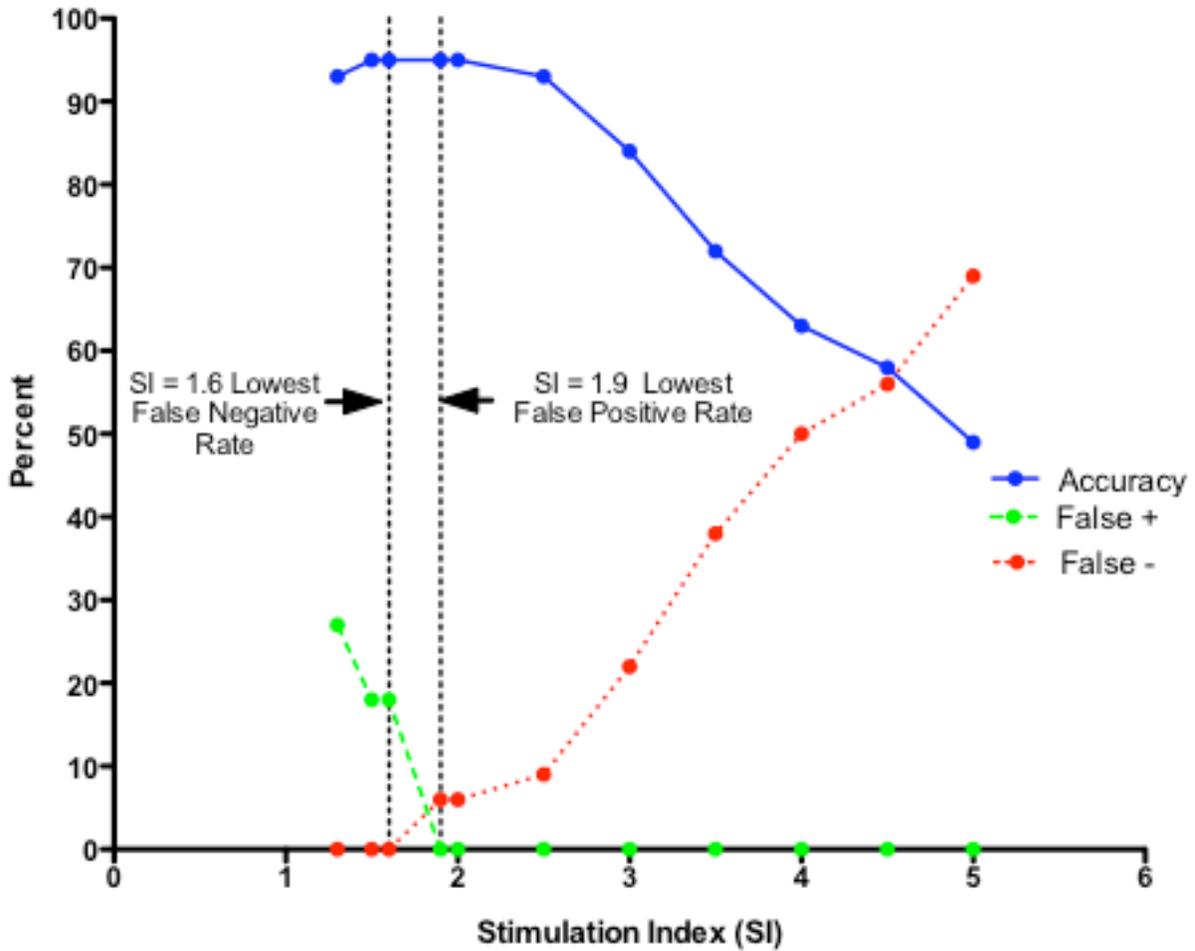


Compared to traditional LLNA results, the lines show the change in performance characteristics for the LLNA: BrdU-ELISA with the SI used to identify skin sensitizers. This analysis used LLNA results for 32 sensitizers and 11 nonsensitizers. For 18 substances with multiple LLNA: BrdU-ELISA test results, the most prevalent outcome was used.

LLNA:BrdU-ELISA Test Method Usefulness and Limitations

- The LLNA: BrdU-ELISA can be used to identify potential skin sensitizers or nonsensitizers.
 - Use $SI \geq 1.6$ to identify potential skin sensitizers.
- A slight potential for false positives with borderline weak positive responses ($1.6 < SI < 1.9$) exists.
 - Consider additional information such as dose-response relationship strength, statistical significance, evidence of systemic toxicity, and/or excessive skin irritation together with SI values.
- The LLNA: BrdU-ELISA might not be appropriate for testing classes of materials with properties that interfere with the assay.
 - Unlike the traditional LLNA, the LLNA: BrdU-ELISA can be used to test nickel compounds, based on its ability to correctly identify these compounds as potential skin sensitizers.

LLNA Peer Review Panel Meetings

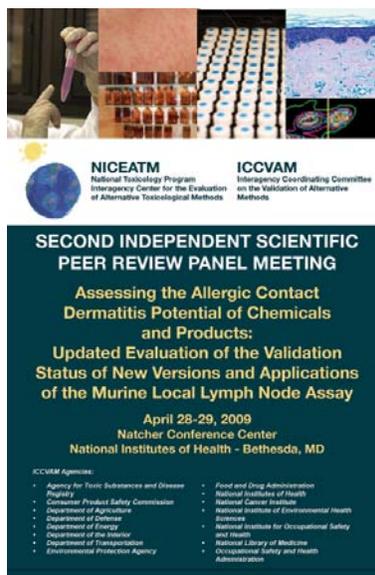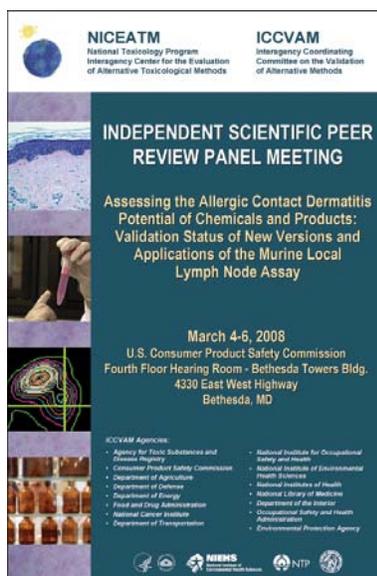

- Public meetings of an international independent scientific peer review panel were held at the Consumer Product Safety Commission in Bethesda, MD, on March 4-6, 2008, and at the National Institutes of Health in Bethesda, MD, on April 28-29, 2009.

Charge to the Peer Review Panel

- Review the draft Background Review Document (BRD) for errors and omissions
- Provide conclusions and recommendations on the current validation status of the LLNA: BrdU-ELISA
- Does the information contained in the draft BRD support ICCVAM's draft test method recommendations?

Peer Review Panel Conclusions

- Concurred that the available data and test method performance supported the use of the LLNA: BrdU-ELISA to identify substances as sensitizers and nonsensitizers, with certain limitations
- Recommended that before animal testing is conducted, consideration be given to the necessity for the substance to be tested for skin sensitization potential
- The complete LLNA Peer Review Panel Reports can be accessed at:
 - http://iccvam.niehs.nih.gov/docs/immunotox_docs/LLNAPRPRpt2008.pdf
 - http://iccvam.niehs.nih.gov/docs/immunotox_docs/LLNAPRPRpt2009.pdf

Independent Scientific Peer Review Panel

Michael Luster, PhD (Panel Chair)

Senior Consultant to the National
Institute for Occupational Safety and
Health
Morgantown, WV

Nathalie Alépée, PhD

L'Oréal Research and Development
Aulnay sous Bois, France

Anne Marie Api, PhD

Research Institute for Fragrance
Materials
Woodcliff Lake, NJ

Nancy Flournoy, MS, PhD

University of Missouri–Columbia
Columbia, MO

Thomas Gebel, PhD

Federal Institute for Occupational Safety
and Health
Dortmund, Germany

Sidney Green, PhD

Howard University
Washington, DC

Kim Headrick, BAdmin, BSc

Health Canada
Ottawa, Ontario, Canada

Dagmar Jírová, MD, PhD

National Institute of Public Health
Prague, Czech Republic

David Lovell, PhD

University of Surrey
Guildford, Surrey, U.K.

Howard Maibach, MD

University of California–San Francisco
San Francisco, CA

James McDougal, PhD

Wright State University
Dayton, OH

Michael Olson, PhD

GlaxoSmithKline
Research Triangle Park, NC

Raymond Pieters, PhD

Utrecht University
Utrecht, The Netherlands

Jean Regal, PhD

University of Minnesota Medical School
Duluth, MN

Jonathan Richmond, MB ChB, FRCSEd

Home Office
London, U.K.

Peter Theran, VMD

Consultant, Massachusetts Society for
the Prevention of Cruelty to Animals
Novato, CA

Stephen Ullrich, PhD

M.D. Anderson Cancer Center
Houston, TX

Michael Woolhiser, PhD

Dow Chemical
Midland, MI

Takahiko Yoshida, MD, PhD

Asahikawa Medical College
Hokkaido, Japan



International Acceptance of the LLNA: BrdU-ELISA

- ICCVAM agreed with the OECD Expert Consultation Group that a single $SI \geq 1.6$ to classify substances as skin sensitizers would avoid false negative and indeterminate results, which are not useful for regulatory purposes.
- OECD Test Guideline 442B Skin Sensitization: Local Lymph Node Assay: BrdU-ELISA, which includes the $SI \geq 1.6$ to classify substances as skin sensitizers, was adopted on July 22, 2010 (OECD 2010).
- OECD Test Guideline 442B can be accessed at <http://www.oecd-ilibrary.org/>
- International acceptance of the LLNA: BrdU-ELISA is expected to result in broader use of LLNA tests.
 - Will further reduce and refine animal use for ACD hazard assessments on a global basis, while ensuring human safety
 - Will reduce costs and environmental hazards associated with the use of radioactive substances

ICCVAM Interagency Immunotoxicity Working Group

Consumer Product Safety Commission

Joanna Matheson, PhD (Working Group Co-
chair)
Marilyn Wind, PhD (to July 2010)

Environmental Protection Agency

Office of Pesticide Programs

Jonathan Chen, PhD
John R. "Jack" Fowle III, PhD, DABT
Masih Hashim, DVM, PhD
Marianne Lewis
Deborah McCall
Timothy McMahon, PhD
John Redden
Jenny Tao, PhD

Office of Pollution Prevention and Toxics

Elizabeth Margosches, PhD
Ronald Ward, PhD

Office of Research and Development

Marsha Ward, PhD

Food and Drug Administration

Center for Devices and Radiological Health

Vasant G. Malshet, PhD, DABT
Jeffrey Toy, PhD

Center for Drug Evaluation and Research

Ruth Barratt, PhD, DVM
Paul Brown, PhD
Abigail Jacobs, PhD (Working Group Co-
chair)
Jiaqin Yao, PhD

Center for Food Safety and Applied Nutrition

Donnie Lowther
Neil Wilcox, DVM, MPH (to April 2011)

Office of the Commissioner

Suzanne Fitzpatrick, PhD, DABT

National Institute of Environmental Health Sciences

Warren Casey, PhD, DABT
Dori Germolec, PhD
William Stokes, DVM, DACLAM

National Institute for Occupational Safety and Health

B. Jean Meade, DVM, PhD
Paul D. Siegel, PhD

National Library of Medicine

Pertti Hakkinen, PhD

European Centre for the Validation of Alternative Methods - Liaison

Silvia Casati, PhD
Alexandre Angers, PhD

Japanese Center for the Validation of Alternative Methods - Liaison

Hajime Kojima, PhD

References

ESAC. 2007. ESAC statement on the reduced local lymph node assay. ECVAM, Joint Research Centre, Institute for Health and Consumer Protection.

ICCVAM. 2009. ICCVAM Test Method Evaluation Report. The Reduced Murine Local Lymph Node Assay: An Alternative Test Method Using Fewer Animals to Assess the Allergic Contact Dermatitis Potential of Chemicals and Products. Available at:

<http://iccvam.niehs.nih.gov/methods/immunotox/LLNA-LD/TMER.htm>.

Kimber I, et al. 2006. Contact Dermatitis 54:181-185.

Kojima H, et al. 2008. Inter-laboratory validation study on LLNA-BrdU [Abstract]. 47th Annual Meeting of the Society of Toxicology.

OECD. 2010. Test No. 442B. Skin Sensitization: Local Lymph Node Assay: BrdU–ELISA. In: OECD Guidelines for the Testing of Chemicals, Section 4: Health Effects. Available at:

http://www.oecd-ilibrary.org/environment/test-no-442b-skin-sensitization_9789264090996-en

Takeyoshi M, et al. 2001. Toxicol Lett 119:203-208.

Takeyoshi M, et al. 2003. Toxicology 191:259-263.

Takeyoshi M, et al. 2004a. J Appl Toxicol 24:77-81.

Takeyoshi M, et al. 2004b. Exp Anim 53:171-173.

Takeyoshi M, et al. 2005. J Appl Toxicol 25:129-134.

Takeyoshi M, et al. 2006. J Appl Toxicol 26:5-9.

Takeyoshi M. 2007. Promising Endpoint and Assay Performance of Non-radioisotopic Local Lymph Node Assay Based on BrdU Incorporation [Abstract]. 6th World Congress on Alternatives & Animal Use in the Life Sciences.

▪

Acknowledgments

The Intramural Research Program of the National Institute of Environmental Health Sciences (NIEHS) supported this poster. Technical support was provided by ILS, Inc., under NIEHS contract N01-ES 35504.

This poster reflects the views of the authors. The views expressed above have not been reviewed or approved by the U.S. Consumer Product Safety Commission or any other U.S. Federal agency and do not necessarily represent the official position of any U.S. Federal agency.

Since the poster was written as part of the official duties of the authors, it can be freely copied. NICEATM and ICCVAM gratefully acknowledge the following individuals and institutions that submitted data to NICEATM used to evaluate the LLNA: BrdU-ELISA.

Masahiro Takeyoshi, PhD
Chemicals Evaluation and Research
Institute
Saitama, Japan

Hajime Kojima, PhD
Japanese Center for the Validation of
Alternative Methods
National Institute of Health Sciences
Ministry of Health, Labour and Welfare
Tokyo, Japan