

Adaptation of the BG1Luc Estrogen Receptor Transactivation Test Method to qHTS: Comparison of Results from Both Methods


Abstract

In 2011, the National Toxicology Program Interagency Center for the Evaluation of Alternative Toxicological Methods nominated the BG1Luc estrogen receptor (ER) transactivation (TA) test method (BG1Luc ER TA) to Tox21 to be adapted into a quantitative high-throughput screening (gHTS) format. The Tox21 collaboration, an effort by the National Toxicology Program, NIH Chemical Genomics Center, Environmental Protection Agency, and Food and Drug Administration, was formed to advance toxicity testing by shifting from traditional *in vivo* tests to *in vitro* methods. A major goal of Tox21 is to prioritize chemicals for in-depth toxicity testing. One approach for prioritization is to use qHTS celland biochemical-based assays to construct concentration-response curves for thousands of chemicals. The Tox21 consortium adapted the BG1Luc ER TA method to a qHTS format. Data were generated for approximately 10,000 chemicals with both the agonist and antagonist versions of the qHTS method. Seventy-six chemicals were tested with both the BG1Luc ER TA manual and gHTS methods. These data were used to evaluate the degree to which classifications of test chemicals with the manual and gHTS methods matched the classifications for performance standards (accuracy) and the degree to which the classifications were identical between the two methods (concordance). Agonist and antagonist methods produced 97% to 100% accuracy and 93% to 96% concordance, respectively, demonstrating that the performance of the gHTS format is comparable to that of the validated BG1Luc ER TA method. (ILS staff supported by NIEHS contract N01-ES 35504.)

Introduction

- The LUMI-CELL[®] BG1Luc4E2 estrogen receptor (ER) transactivation (TA) test method (BG1Luc ER TA) detects estrogen receptor agonists and antagonists.
- The method uses BG-1Luc4E2 cells (Rogers and Denison 2000):
- An immortalized human ovarian adenocarcinoma cell line
- Stably transfected with an estrogen-responsive luciferase reporter gene
- Measures TA via ER-mediated pathways (Figure 1).



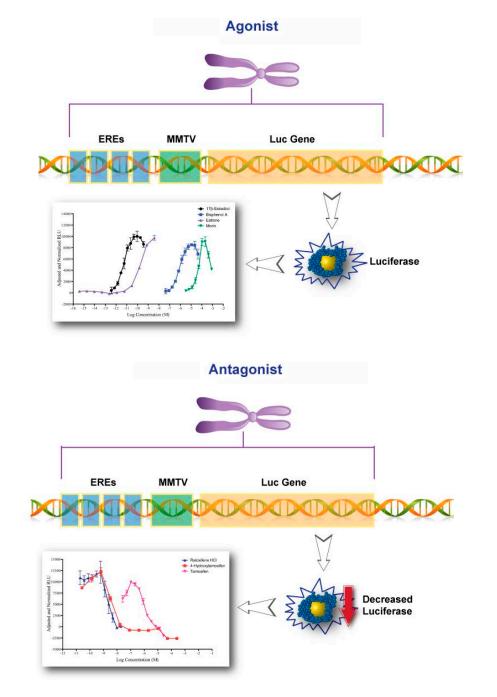

Adaptation of the BG1Luc ER TA Manual Method to qHTS

- Adaptation to gHTS was conducted in a phased approach.
- Methods submitted to Tox21 must be adapted to a 1536-well format.
- Guidance criteria for Tox21 assays are listed on the NCATS website:
- http://www.ncats.nih.gov/research/reengineering/ncgc/assay/criteria/criteria.html.
- Tox21 assays are evaluated using a small library such as the Sigma-Aldrich Library of Pharmacologically Active Compounds, run in triplicate (NTP 2010).
- Assay acceptance criteria include a Z factor (Zhang 1999) greater than 0.5, a coefficient of variation less than 10%, and a signal-tobackground ratio larger than 3 (NTP 2010).
- Assays that meet these acceptance criteria are used to test the Tox21 10,000-chemical library.
- Having met these performance criteria, the BG1Luc ER TA (BG1) gHTS method was then considered to be adapted for Tox21.

Table 1. Comparison of BG1Luc ER TA Manual and **qHTS Methods**

BG1 Manual	BG1 qHTS
Hand pipetted	Fully automated
96-well plate	1536-well plate
2 test substances per plate	1408 test substances per plate
11 test substance concentrations per plate	One test substance concentration per plate
Complete concentration- response curve for each substance on a single plate	Complete concentration- response curve generated over 15 test plates
Concentrations determined by range finder, followed by focused testing (~3 log range) up to the limit of solubility or 1 mM	Fixed concentrations typically ranging from 0.5 nM to 92 μM
Each test substance tested in triplicate in each experiment	Each test substance tested once in each experiment
Each experiment performed at least twice (OECD 2012a,b)	Each experiment performed in triplicate
40,000 cells per well	4000 cells per well
200 µL per well	10 µL per well
Wash steps	No wash steps
7 to 14 days	3 days
Viability determined visually	Viability determined by fluorescence

- simultaneously by testing 10 sets of 15 test plates (Inglese 2006) for a total of 150 plates per experiment.
- Each experiment is repeated in three independent runs.
- The complete set of 10,000 Tox21 chemicals was screened using the BG1 qHTS method.
- Data analyses are ongoing.
- Seventy-six chemicals were tested with both the BG1 manual and qHTS methods, allowing for comparison of data between methods.

P Ceger¹, J Strickland¹, L Rinckel¹, W Casey²; ¹ILS, Inc., RTP, NC, USA; ²NICEATM/NTP/HHS, RTP, NC, USA

Figure 2. BG1 qHTS Test Plate Layout


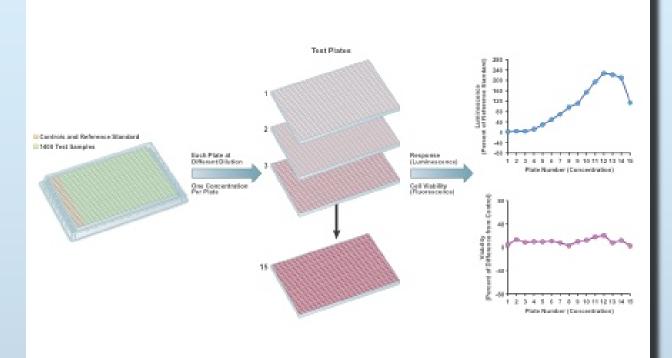


Figure represents one set of 15 plates.


Data Analysis Methods

- Concentration-response curves were graphed for each substance. A positive, negative, or inconclusive classification was assigned to each graph.
- The BG1 gHTS data were graphed for comparison to the BG1 manual method (Figures 3 and 4).
- Each graph was evaluated and assigned a classification of positive. negative, or inconclusive.
- For positive substances, the half-maximal effective concentration (EC_{50}) or the half-maximal inhibitory concentration (IC_{50}) values were calculated using a 4-parameter Hill function.

Figure 3. **Representative Positive Agonist Response** with BG1Luc ER TA Manual and BG1 gHTS Methods: Bisphenol A

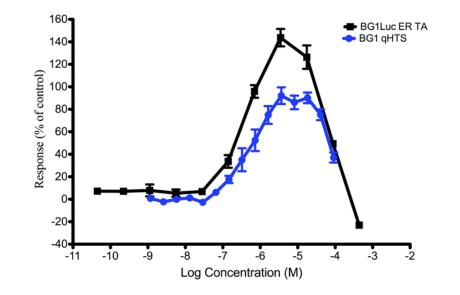

The graph shows concentration-response curves for bisphenol A tested with the agonist protocols for the BG1Luc ER TA manual and qHTS methods. Each data point represents the mean ± standard deviation from the mean for three experiments. These curves were classified as positive

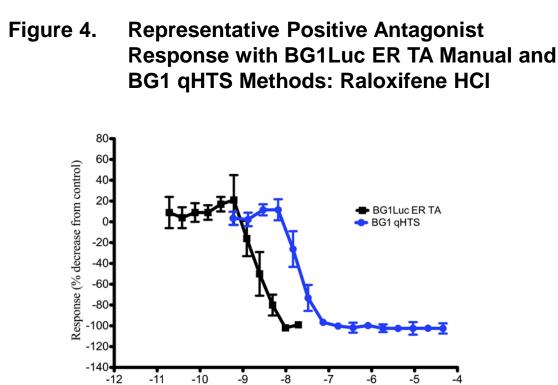

Log Concentration (M)

The graph shows concentration-response curves for raloxifene HCI tested with the antagonist protocols for the BG1Luc ER TA manual and qHTS methods. Each data point represents the mean ± standard deviation from the mean for three experiments. These curves were classified as positive.

Accuracy


Table 2. Accuracy of the Agonist Protocols for the BG1Luc ER TA Manual and gHTS Methods

	BG1 Manual	BG1 qHTS	
Positive 27		26	
Negative 7		7	
Overall	34/34 (100%)	33/34 (97%)	

	BG1 Manual BG1 qH		
Positive 3		3	
Negative	Negative 22		
Overall	25/25 (100%)	25/25 (100%)	

- aHTS methods.
- (**Figures 5** and **6**).

Figure 5.

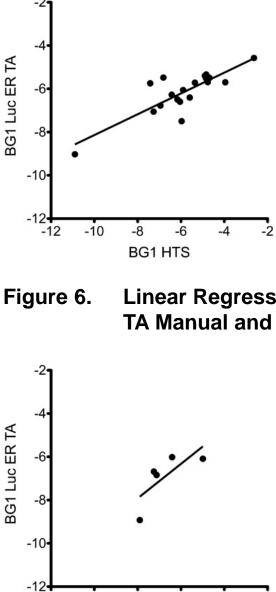

Accuracy and Concordance

 ICCVAM developed performance standards for the BG1Luc ER TA manual method to evaluate the comparability of proposed test methods that are functionally and mechanistically similar (ICCVAM 2011). The performance standards include a minimum list of reference substances for assessing the accuracy of the proposed test method (42 for agonists; 25 for antagonists).

 Accuracy was determined for both test methods using the reference substances from the ICCVAM performance standards.

- Substances that were classified as inconclusive with either method were omitted from analysis.

> Agonist accuracy was calculated for 34 substances (27 positive, 7 negative). Accuracy for the BG1 manual method was 100% (34/34). • Accuracy for the BG1 gHTS method was 97% (33/34).

Table 3. Accuracy of the Antagonist Protocols for the **BG1Luc ER TA Manual and gHTS Methods**

 Antagonist accuracy was calculated for 25 substances (3 positive, 22 negative). Accuracy for both methods was 100% (25/25).

• An EC₅₀ or IC₅₀ value was calculated for all positive substances from the concentration-response curves for the BG1 manual and

• Linear regression analysis was used to compare the two value sets

Linear Regression Analysis of BG1Luc ER TA Manual and qHTS EC₅₀ Values

- The line represents the linear regression through those EC₅₀ values.
- The slope of the linear regression line is 0.48, r² is 0.69.

Linear Regression Analysis of BG1Luc ER TA Manual and qHTS IC₅₀ Values

- The line represents the linear regression through those IC₅₀
- The slope of the linear regression line is 0.80, r² is 0.56.

Accuracy and Concordance (cont'd)

Concordance

- The results from the 76 chemicals tested with both methods were evaluated for concordance.
- Substances that were classified as inconclusive with either method were omitted from analysis.

Table 4. Concordance of the Agonist Protocols for the **BG1Luc ER TA Manual and gHTS Methods**

	BG1 qHTS Classification			
ual ion		Positive	Negative	Total
BG1 Manual Classificatior	Positive	31	4	35
31 N Issif	Negative	0	26	26
BC	Total	31	26	61

- Concordance was calculated for 61 substances (35 positive, 26 negative).
- Concordance between the BG1 manual and BG1 gHTS methods was 93% (57/61).

Table 5. Concordance of the Antagonist Protocols for the BG1Luc ER TA Manual and gHTS Methods

	BG1 qHTS Classification			
al on		Positive	Negative	Total
lanu icati	Positive	6	3	9
BG1 Manual Classification	Negative	0	64	64
BG Cla	Total	6	67	73


 Concordance was calculated for 73 substances (9 positive, 64 negative)

 Concordance between the BG1 manual and BG1 qHTS methods was 96% (70/73).

Discussion


- Accuracy was determined by comparing the results from each method with ICCVAM reference classifications for the 34 substances used to evaluate agonists and the 25 substances used to evaluate antagonists. Performance standards include reference substances that are recommended for evaluating functionally and mechanistically similar test methods (ICCVAM 2011).
- Using the performance standards, the accuracy of the BG1 qHTS was nearly identical to that of the BG1 manual method and provided comparable EC_{50} and IC_{50} values.
- Concordance between the two methods was high, with the few discrepancies appearing to be related primarily to differences in the upper limit of testing concentrations (see **Figures 7** and **8** for examples).

Discordant Agonist Response with BG1Luc Figure 7. ER TA Manual and gHTS Methods: Phenolphthalein




- Each data point represents the mean ± standard deviation from the mean for three experiments. The BG1Luc ER TA manual curve was classified as positive: the BG1 qHTS curve was classified as negative.
- The dashed line indicates the highest concentration tested with the BG1 gHTS method
- · Increased variability among the three experimental replicates indicates that the test substance tested positive in at least one experiment
- A general upward trend suggests that this substance would test positive with the BG1 gHTS method if tested at higher concentrations

Discordant Antagonist Response with Figure 8. **BG1Luc ER TA Manual and gHTS Methods:** Medroxyprogesterone acetate

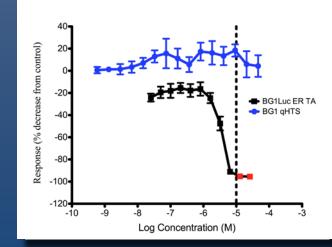

- Each data point represents the mean ± standard deviation from the mean for three experiments. Points highlighted in red indicate where cytotoxicity likely impacted the response. The BG1Luc ER TA manual curve was classified as positive; the BG1 gHTS curve was classified as negative.
- Antagonist substances that show a decrease in response only at concentrations greater than 10 µM (vertical dashed line) are considered negative (ICCVAM 2011).



Conclusions

- Accuracy for the BG1 gHTS was nearly identical to that of the BG1 manual method (97% [33/34] and 100% [25/25] for the agonist and antagonist protocols, respectively), with comparable EC_{50} and IC_{50} values.
- Concordance between the BG1 manual and gHTS methods was 93% (57/61) and 96% (70/73) for the agonist and antagonist protocols, respectively. The few discordant values with the BG1 qHTS method were due to negative results for substances that tested positive with the BG1 manual method and may be attributed to lower maximum concentrations tested with for the aHTS method
- The BG1 gHTS has performed well for a subset of ICCVAM reference substances.

References

ICCVAM. 2011. ICCVAM Test Method Evaluation Report. The LUMI-CELL® ER (BG1Luc ER TA) Test Method: An In Vitro Assay for Identifying Human Estrogen Receptor Agonist and Antagonist Activity of Chemicals. NIH Publication No. 11-7850. Research Triangle Park, NC:National Institute of Environmental Health Sciences.

Inglese J, Auld DS, Jadhav A, Johnson RL, Simeonov A, Yasgar A, et al. 2006. Quantitative highthroughput screening: a titration-based approach that efficiently identifies biological activities in large chemical libraries. Proc Natl Acad Sci USA103(31): 11473-11478.

NTP. 2010. Review of the Biomolecular Screening Branch by the NTP Board of Scientific Counselors. Research Triangle Park, NC:National Toxicology Program.

OECD. 2012a. Test No. 455. Performance-Based Test Guideline for Stably Transfected Transactivation In Vitro Assays to Detect Estrogen Receptor Agonists [adopted 2 October 2012]. In: OECD Guidelines for the Testing of Chemicals, Section 4: Health Effects. Paris:OECD Publishing.

OECD. 2012b. Test No. 457. BG1Luc Estrogen Receptor Transactivation Test Method for Identifying Estrogen Receptor Agonists and Antagonists [adopted 2 October 2012]. In: OECD Guidelines for the Testing of Chemicals, Section 4: Health Effects. Paris:OECD Publishing.

Rogers JM, Denison MS. 2000. Recombinant cell bioassays for endocrine disruptors: development of a stably transfected human ovarian cell line for the detection of estrogenic and anti-estrogenic chemicals. In Vitr Mol Toxicol 13(1): 67-82.

Zhang JH, Chung TD, Oldenburg KR. 1999. A simple statistical parameter for use in evaluation and validation of high throughput screening assays. J Biomol Screen 4(2): 67-73.

Acknowledgements

The Intramural Research Program of the National Institute of Environmental Health Sciences (NIEHS) supported this poster. Technical support was provided by ILS, Inc., under NIEHS contract N01-ES 35504.

The views expressed above do not necessarily represent the official positions of any Federal agency. Since the poster was written as part of the official duties of the authors, it can be freely

